



PROCEEDINGS

Open Access

Study of parameters in focus simulation functions of virtual slide

Ichiro Mori*, Takashi Ozaki, Emiko Taniguchi, Kennichi Kakudo

From The 10th European Congress on Telepathology and 4th International Congress on Virtual Microscopy Vilnius, Lithuania. 1-3 July 2010

Abstract

As a special function of Virtual Slide (VS) for thick specimens like cytology slides, multilayer (Z-stack) simulated focus and focus fusion were introduced. From the standpoint of surgical pathologist, the optimum parameters for multilayer focus simulation were examined. First, minimal thickness of the layer was checked by measuring thickness of small cells counting the number of the layers that come into focus. Then the optimal number of layers to scan, total thickness, was tried. Small-sized cell nuclei showed around 2 μ m or less thickness. As minimal thickness of one layer for focus simulation, less than 2 μ m is required. Papillary cell mass of urothelial carcinoma, aspiration cytology specimen of breast or thyroid, and uterine cervical smear showed different optimal thickness. Cells piling up more than 4 to 5 layer are difficult to make close up observation. Total 15 (to 30) μ m thick scan was enough for most specimens. The "focus fusion" image is single layer image synthesized from multiple layer images. Several layer thicknesses were examined, and there was negligible difference between the focus fusion image synthesized from 0.25 and 1 μ m thick layers. In the focus fusion image synthesized from 3 μ m thick layers, some cells not to come into focus. The "focus fusion" seems to contain all the cells in one plane, and easy for screening. To emphasize the existence of myoepithelial cells in fibroadenoma of breast, or to clarify the 3-dimensional tissue structure, multilayer image was better. From our results, 10 layers with 1.5 μ m thick each provide sufficient information in most specimens.

Introduction

Virtual slide technology is now introduced to many fields[1-5]. Among these, cytology slide diagnosis is remaining as a big challenge because it requires focus control and high resolution[6]. Focus simulation using multilayer or Z-stack and focus fusion were introduced in late years. Our aim is to decide the optimal parameters for focus simulation functions, the thickness of each layer and how many layers should we cut.

Material and methods

The virtual slide scanner we used is TOCO from Claro, the tiling type scanner that has multilayer and focus fusion function (Figure 1). The nuclear width was measured using scale bar on the screen provided by virtual

slide viewer. The thickness of the nuclei was measured by counting the layers that come into focus. The viewer has button to change focus planes with one click for one layer. At least ten cells were count.

To decide the optimum layer thickness for multilayer focus simulation, we should know whether the cells in cytology slide keeps 3-dimensional shape or deformed by preparation procedure. We tried to check the 3-D shape of lymphocyte nuclei using formalin-fixed, paraffin section because the paraffin section is expected to keep original nuclear shape. We made 10 μ m thick paraffin section of spleen from an autopsy case, and then scanned with layers of 0.25 μ m thick each. We carefully select lymphocytes that has whole nucleus in the 10 μ m section, then count the number of layers that come into focus.

Next, we checked the 3-D shape of lymphocyte nuclei in thick cytology specimen. Lymphocytes in breast aspiration cytology specimen were measured. We also

* Correspondence: ichiro-m@wakayama-med.ac.jp
Department of Human Pathology, Wakayama Medical University 811-1,
Kimiidera, Wakayama City, Wakayama 641-8509, Japan
Full list of author information is available at the end of the article

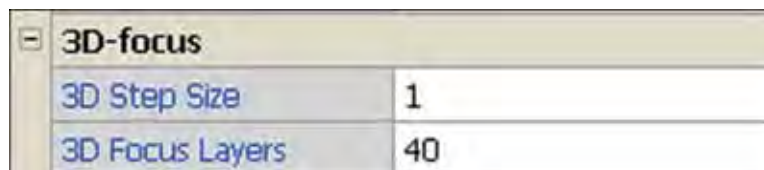


Figure 1 Focus simulation control menu. "3D Step Size" sets layer thickness with value "1" for 0.25µm. "3D Focus Layers" sets the total number of layers with value "40" for 40 layers on both side of autofocus plane. This setting, 3D Step Size: 1 and 3D Focus Layers: 40, results 0.25 X (40+1 +40), almost 20µm as total thickness to scan.

checked lymphocytes in Giemsa slide that uses drying fixation and improperly dried lymphocytes in Papanicolaou slides.

Then the 3-D shape of various cells was measured. We measured nuclei of myoepithelial cells and duct epithelial cells from the breast fibroadenoma specimen together with the distance between these cells. Small-sized cells like surface squamous epithelial cells and shrunk cells in urine were also measured. Based on these data, optimal layer thickness is considered.

To decide the total thickness to scan, thick specimens like papillary cell mass of urothelial carcinoma, aspiration cytology specimen of breast or thyroid were selected, and tried to decide how many stacked nuclei are possible to diagnose.

In "focus fusion" image, the same layer thickness is possible to indicate. Several layer thicknesses were examined.

Results

The lymphocyte nuclei in the paraffin section of spleen have 4.3 to 4.5µm diameter, and 16 to 20 layers thickness, that correspond approximately to 4 to 5µm thickness. Lymphocyte nuclei in the thick breast aspiration cytology specimen have diameter of about 4.7 to 5.4µm, and 16 to 20 layers that correspond to 4 to 5µm. In the months-old slides, the lymphocyte nuclei showed similar diameter, but the thickness decreased to about 2 to 3µm. We checked Giemsa slide that uses drying fixation and improperly dried cells in Papanicolaou slides. The lymphocyte nuclei were flattened to 1.25 to 2.5µm (Table 1).

Next, we measured myoepithelial cells from the breast fibroadenoma. The myoepithelial cell nuclei had rugby ball-like shape with longer axis for 5.9 to 7.5µm and shorter axis for 2.2 to 3.2µm. Nuclear thickness was

Table 1 Nuclear size of lymphocyte

	Diameter	Thickness
Spleen (Formalin-fixed paraffin section)	4.3 - 4.5	4 - 5
Breast (aspiration cytology)	4.7 - 5.4	4 - 5
Giemsa (pleural effusion)	5.1 - 6.4	1.25 - 1.5

about 2.0 to 2.5µm. The duct epithelial cell nuclei of the same breast fibroadenoma showed fried egg-like shape with 6.8 to 8.5µm diameter and 2.0 to 3.0µm thickness (Table 2).

The depth direction distance between myoepithelial cells and duct epithelial cells was measured counting the layers between the myoepithelial cell nuclei's largest diameter to the duct epithelial cell nuclei's largest diameter, which was about 2.5 to 3µm. Figure 2 shows schematic side view of these breast duct cells in scaled size.

As far we tried, more than 5 to 6 nuclei stacked together was difficult to distinguish, and not good for diagnosis use. Total thickness to scan also depends on the size of the nuclei. The largest nucleus we found in this study was urothelial carcinoma cell in urine that has 50µm diameter and about 10µm thickness.


Using the "focus fusion", several layer thicknesses were examined, and there was negligible difference between the focus fusion image synthesized from 0.25 and 1µm thick layers. In the focus fusion image synthesized from 3µm thick layers, some cells occasionally disappears or not to come into focus.

Discussion

Using scale bar on the screen for diameter, and count the layers that come into focus for the thickness, the lymphocyte nuclei in formalin-fixed, paraffin section showed almost spherical shape. This result assures that we can use our virtual slide in semi-morphometrical analysis. Then we measured lymphocyte nuclei in thick cytology slide, and found that they also keep spherical shape still after embedding in the medium. Nuclear

Table 2 Nuclear size of various cells

	Diameter (long)	Diameter (short)	Thickness
Myoepithelial cell nuclei	5.9 - 7.5	2.2 - 3.2	2.0 - 2.5
Duct epithelial cell nuclei	6.8 - 8.5	6.8 - 8.5	2.0 - 3.0
Surface squamous epithelial cell	4.4 - 4.7	4.4 - 4.7	1 - 1.25
Middle squamous epithelial cells	8.5 - 10.1	6.4 - 7.2	2.0 - 2.5
Urothelial cells	5.4 - 8.5	4.4 - 5.4	2.0 - 4.25

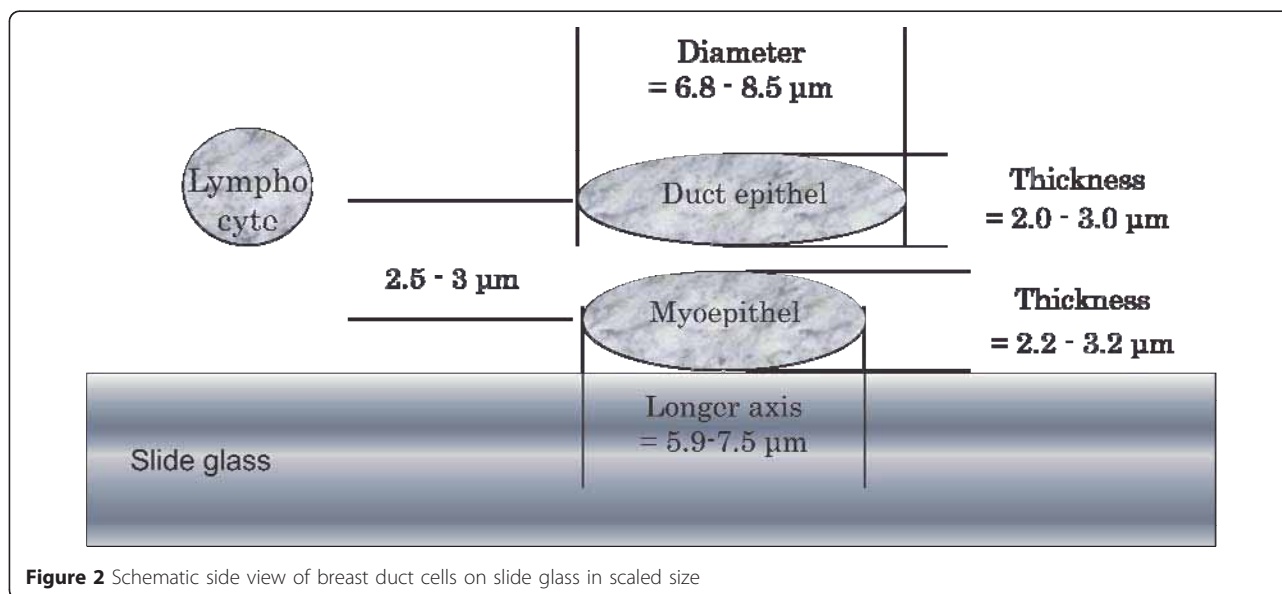

size was about 4 to 5 μm , smaller than the value shown in histology textbook (6 to 15 μm)[7]. This result is possibly due to preparation procedure. Histological slide suffered formalin fixation and heat coagulation in melted paraffin, and cytological slide suffers alcoholic fixation. In the months-old slides, the nuclei diameter was nearly the same, but the thickness got flat to about 2 to 3 μm . This result is probably due to drying of mounting medium. Lymphocytes in air-dried Giemsa slide and improperly dried cells in Papanicolaou slides were highly flattened.

Small-sized cells like myoepithelial cells of breast duct, surface squamous epithelial cells, and shrunk cells in urine showed around 2 μm thickness. If these cell mass is cut into 2 μm layers, some of the nuclei may not come into focus on the virtual slide. Less than 2 μm layer thickness is required for focus simulation. Thinner layer results fine pictures, but the thinner the layer set, the more the total number of layers increase. This causes longer scan time, more data size, and slower response to observe.

Thinking about total thickness to scan, number of stacked nuclei and the nuclear size should be considered. Papillary cell mass of urothelial carcinoma, aspiration cytology specimen of breast or thyroid, and uterine cervical smear showed different optimal thickness. Using our virtual slide, nuclei stacked more than 5 to 6 layers was difficult to distinguish. Stacked 5 nuclei of 2 μm thickness each results in 10 μm to scan. But usually carcinoma cells have big nuclei, as big as 50 μm diameter and 10 μm thickness. If these big cells stack together, we need to scan to 50 μm or more. Usually, slides with more than 5 stacked cancer cell nuclei are exceptional and focal.

The “focus fusion” seems to contain all the cells in one plane, and easy for screening. But when trying to obtain detailed pictures like existence of myoepithelial cells, very important benign sign of breast, or to clarify the 3-dimensional tissue structure, multilayer image was better.

The efficiency of multilayer focus simulation depends on how easy we can change focus. The method to change focus differs from company to company[8]. Too many layer causes slow response. From these findings, we conclude 10 to 15 layers with 1.5 μm thick each provide sufficient information in most specimens. In case of thick slide, 30 μm thick scan may require.

Conclusions

Cells in the cytology slides were smaller than the description in textbook. Layers of 1.5 μm thickness each with total 10 to 15 layers resulting 15 to 20 μm scan is suitable for most cytology slides.

Acknowledgements

This article has been published as part of *Diagnostic Pathology* Volume 6 Supplement 1, 2011: Proceedings of the 10th European Congress on Telepathology and 4th International Congress on Virtual Microscopy. The full contents of the supplement are available online at <http://www.diagnosticpathology.org/supplements/6/S1>

Competing interests

The authors declare that they have no competing interests.

Published: 30 March 2011

References

1. Toyoda Y: Virtual slide scanner corresponding to Fluorescent microscopy and Z-stack picture acquisition [Japanese]. *Abstract Journal of 6th General Meeting of the Japanese Research Society of Telepathology and Pathology Informatics* Yonago; 2007.

2. Saito K, Hayashi H: **Introduction of virtual slide in hospital system [Japanese]**. *Medical Technology* 2008, **36**(8):808-812.
3. Washiya K: **Application of virtual slide to diagnosis use [Japanese]**. *Medical Technology* 2008, **36**(8):828-831.
4. Hashiguchi A, Takechi K, Sakamoto M: **Application of virtual slide to medical student education [Japanese]**. *Medical Technology* 2008, **36**(8):813-817.
5. Uzuki M, Sawai T: **Issues of today's virtual slide and future development [Japanese]**. *Medical Technology* 2008, **36**(8):835-838.
6. Mori I, Nunobiki O, Ozaki T, Taniguchi E, Kakudo K: **Issues for application of virtual microscopy to cytoscreening, perspectives based on questionnaire to Japanese cytotechnologists**. *Diagnostic Pathology* 2008, **3**(Suppl 1):S15.
7. Ross M, Pawlina W: **Histology, A text and atlas, with correlated cell and molecular biology**. Lippincott Williams & Wilkins, Fifth.
8. Mori I, Ozaki T, Taniguchi E, Kakudo K: **Issues for virtual slide diagnosis, integration of manipulation and role sharing with pathology diagnosis support system and electronic clinical record [Japanese]**. *Japanese Journal of Telemedicine and Telecare* 2010, **6**(1).

doi:10.1186/1746-1596-6-S1-S24

Cite this article as: Mori et al.: **Study of parameters in focus simulation functions of virtual slide**. *Diagnostic Pathology* 2011 **6**(Suppl 1):S24.

**Submit your next manuscript to BioMed Central
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

